


# Inspection sheet


Date 2001/4/11

Model FT/IR-460  
Serial No. A004060846  
Temperature 14 C  
Humidity Unk %  
Operator JASCO (UK) Ltd  
Total Judgement good

Inspector



Inspection :%T Repeatability

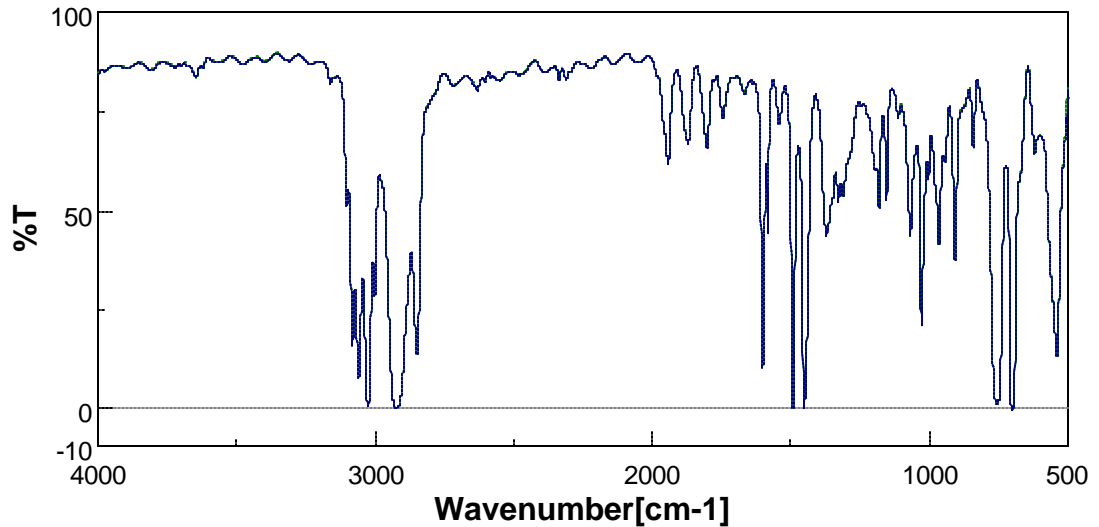

[Standard] +/-0.5 %T (0 - 100%T)

Peak[cm-1]	1st	2nd	Difference	Judgement
2850.70	13.775	13.747	0.027	good
1601.40	10.323	10.303	0.020	good
1583.10	44.244	44.227	0.017	good
1181.40	50.650	50.600	0.050	good
1154.30	52.830	52.781	0.049	good
1069.10	43.677	43.641	0.037	good
1028.00	21.235	21.156	0.080	good
906.70	37.566	37.480	0.087	good