


Inspection sheet



Date 2001/4/11

Model FT/IR-460
 Serial No. A004060846
 Temperature 14 C
 Humidity Unk %
 Operator JASCO (UK) Ltd
 Total Judgement good

Inspector



Inspection :Resolution

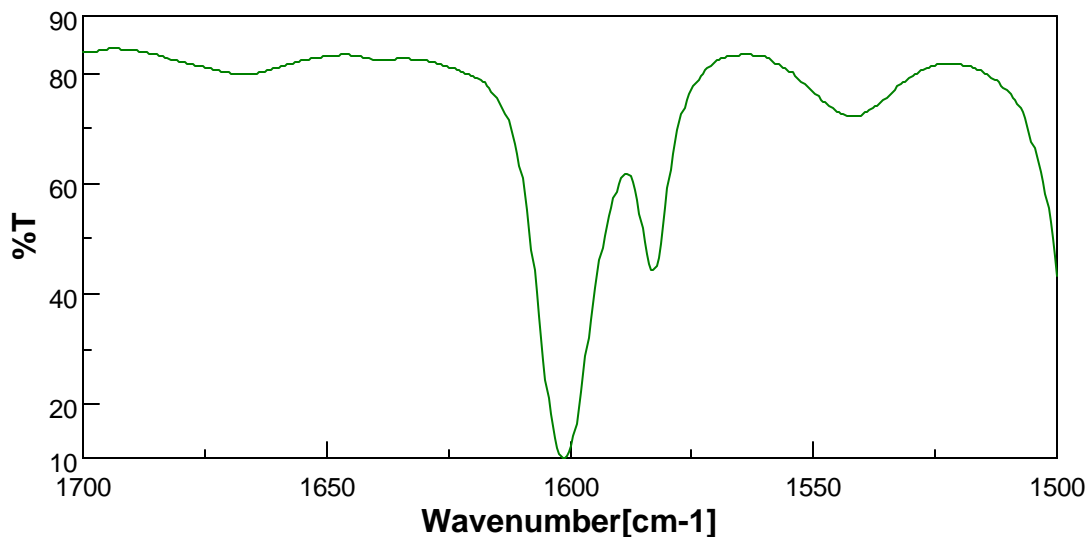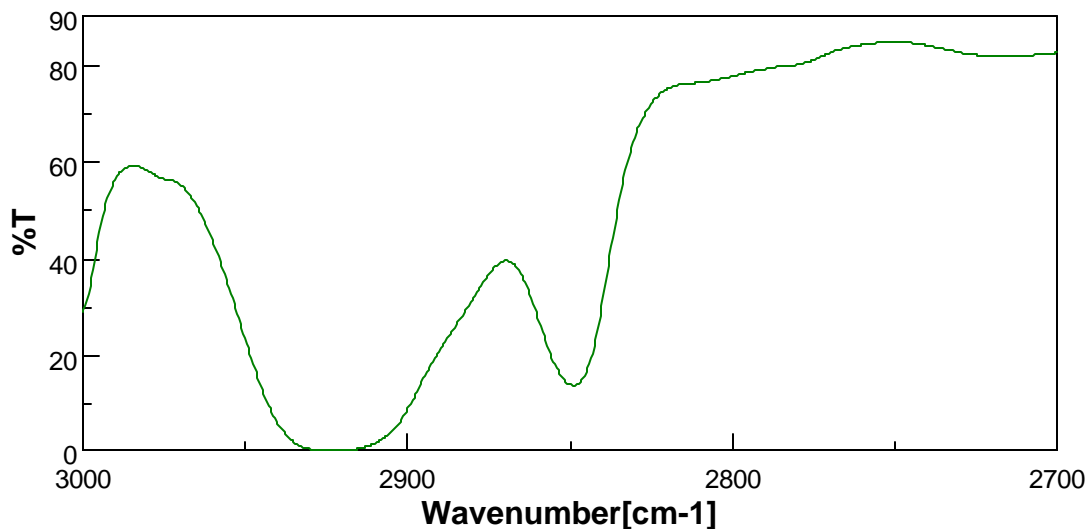

[Standard] Diff.

2851 cm-1 peak no less than 18 %T
 1583 cm-1 peak no less than 10 %T

Peak[cm-1]	%T[valley]	%T[peak]	Difference	Judgement
2848.83	39.631	13.788	25.843	good
1582.79	61.922	44.256	17.666	good